


SM removal/DCM

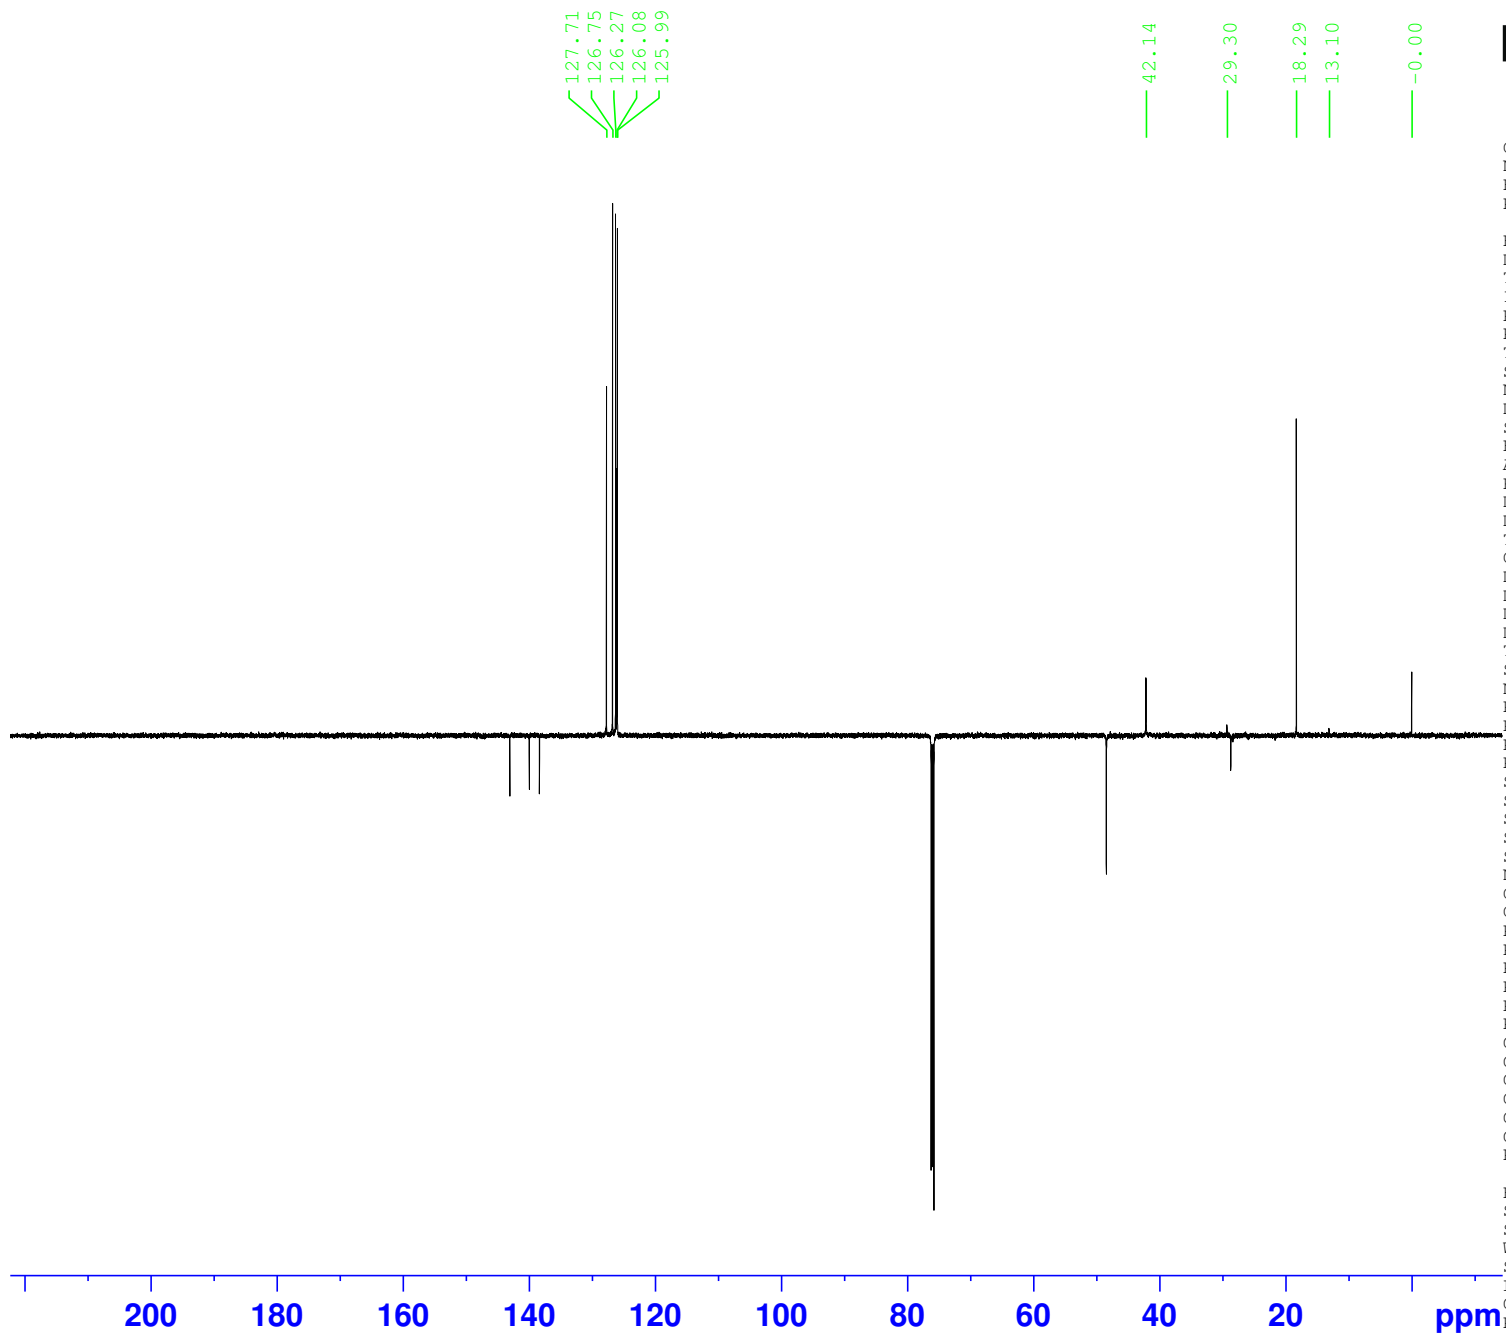

Current Data Parameters
NAME EPW-427a
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240619
Time 13.57 h
INSTRUM spect
PROBHD Z126545_0009 (
PULPROG deptqgppsp
TD 65536
SOLVENT CDC13
NS 512
DS 8
SWH 35714.285 Hz
FIDRES 1.089913 Hz
AQ 0.9175040 sec
RG 194.73
DW 14.000 usec
DE 18.00 usec
TE 298.0 K
CNST2 145.0000000
D1 2.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
D16 0.00020000 sec
TD0 1
SF01 150.9236829 MHz
NUC1 13C
P1 10.00 usec
P13 2000.00 usec
PLW0 0 W
PLW1 58.00000000 W
SPNAM[5] Crp60comp.4
SPOALS 0.500
SPOFFS5 0 Hz
SPW5 8.86170006 W
SF02 600.1524006 MHz
NUC2 1H
CNST12 1.5000000
CPDPRG[2] waltz16
P0 18.00 usec
P3 12.00 usec
P4 24.00 usec
PCPD2 70.00 usec
PLW2 24.71599960 W
PLW12 0.72635001 W
GPNAM[1] SMSQ10.100
GPZ1 31.00 %
GPNAM[2] SMSQ10.100
GPZ2 31.00 %
GPNAM[3] SMSQ10.100
GPZ3 31.00 %
P16 1000.00 usec

F2 - Processing parameters
SI 32768
SF 150.9079936 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40